

IBP Transducer Accessories


HISERN

Interface Cable for IBP Transducer

Hisern Medical offers a wide range configuration of IBP cables that are compatible with patient monitors from major brands. With high quality and durability, the IBP cable enables easy connection between patient monitors and Hisern's IBP transducers.



Cable Connection

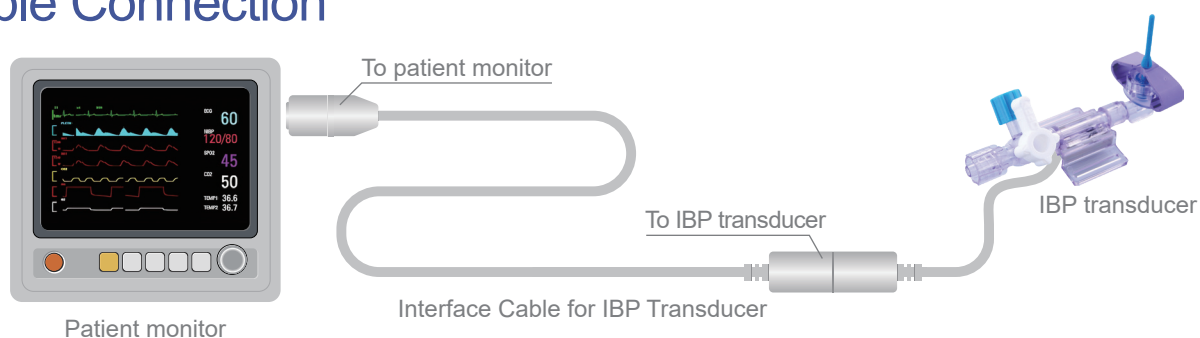

Transducer Connector

We provide 9 types of transducer connectors as following:



Type A



Type B



Type C



Type D



Type E



Type F



Type G



Type H




Type I

Instrument Connector


• For Philips Patient Monitor

PN	Product Description
H02308001	AMD-026A IBP Adapter Cable, Philips 12P to Abbott
H02308002	AMD-026B IBP Adapter Cable, Philips 12P to BD
H02308003	AMD-026E IBP Adapter Cable, Philips 12P to B.Braun
H02308004	AMD-026D IBP Adapter Cable, Philips 12P to Edwards
H02308005	AMD-026C IBP Adapter Cable, Philips 12P to Utah
H02308006	AMD-026F IBP Adapter Cable, Philips 12P to USB





• For GE Patient Monitor

PN	Product Description
H02308007	AMD-062A IBP Adapter Cable, GE 11P to Abbott
H02308008	AMD-062B IBP Adapter Cable, GE 11P to BD
H02308009	AMD-062E IBP Adapter Cable, GE 11P to B.Braun
H02308010	AMD-062D IBP Adapter Cable, GE 11P to Edwards
H02308011	AMD-062C IBP Adapter Cable, GE 11P to Utah
H02308012	AMD-062F IBP Adapter Cable, GE 11P to USB





• For Dräger Patient Monitor

PN	Product Description
H02308013	AMD-003A IBP Adapter Cable, Draeger 7P to Abbott
H02308014	AMD-003B IBP Adapter Cable, Draeger 7P to BD
H02308015	AMD-003E IBP Adapter Cable, Draeger 7P to B.Braun
H02308016	AMD-003D IBP Adapter Cable, Draeger 7P to Edwards
H02308017	AMD-003C IBP Adapter Cable, Draeger 7P to Utah
H02308018	AMD-003F IBP Adapter Cable, Draeger 7P to USB
H02308019	AMD-032A IBP Adapter Cable, Draeger 10P to Abbott
H02308020	AMD-032B IBP Adapter Cable, Draeger 10P to BD
H02308021	AMD-032E IBP Adapter Cable, Draeger 10P to B.Braun
H02308022	AMD-032D IBP Adapter Cable, Draeger 10P to Edwards
H02308023	AMD-032C IBP Adapter Cable, Draeger 10P to Utah
H02308024	AMD-032F IBP Adapter Cable, Draeger 10P to USB
H02308073	AMD-096A IBP Adapter Cable, Draeger 7P to Abbott
H02308074	AMD-096B IBP Adapter Cable, Draeger 7P to BD
H02308075	AMD-096E IBP Adapter Cable, Draeger 7P to B.Braun
H02308076	AMD-096D IBP Adapter Cable, Draeger 7P to Edwards
H02308077	AMD-096C IBP Adapter Cable, Draeger 7P to Utah
H02308078	AMD-096F IBP Adapter Cable, Draeger 7P to USB





• For Nihon Kohden Patient Monitor

PN	Product Description
H02308025	AMD-093A IBP Adapter Cable, Nihon Kohden 14P to Abbott
H02308026	AMD-093B IBP Adapter Cable, Nihon Kohden 14P to BD
H02308027	AMD-093E IBP Adapter Cable, Nihon Kohden 14P to B.Braun
H02308028	AMD-093D IBP Adapter Cable, Nihon Kohden 14P to Edwards
H02308029	AMD-093C IBP Adapter Cable, Nihon Kohden 14P to Utah
H02308030	AMD-093F IBP Adapter Cable, Nihon Kohden 14P to USB
H02308079	AMD-091A IBP Adapter Cable, Nihon Kohden 5P to Abbott
H02308080	AMD-091B IBP Adapter Cable, Nihon Kohden 5P to BD
H02308081	AMD-091E IBP Adapter Cable, Nihon Kohden 5P to B.Braun
H02308082	AMD-091D IBP Adapter Cable, Nihon Kohden 5P to Edwards
H02308083	AMD-091C IBP Adapter Cable, Nihon Kohden 5P to Utah
H02308084	AMD-091F IBP Adapter Cable, Nihon Kohden 5P to USB




• For Mindray Patient Monitor

PN	Product Description
H02308031	AMD-002A IBP Adapter Cable, Mindray 6P to Abbott
H02308032	AMD-002B IBP Adapter Cable, Mindray 6P to BD
H02308033	AMD-002E IBP Adapter Cable, Mindray 6P to B.Braun
H02308034	AMD-002D IBP Adapter Cable, Mindray 6P to Edwards
H02308035	AMD-002C IBP Adapter Cable, Mindray 6P to Utah
H02308036	AMD-002F IBP Adapter Cable, Mindray 6P to USB
H02308037	AMD-357A IBP Adapter Cable, Mindray 12P to Abbott
H02308038	AMD-357B IBP Adapter Cable, Mindray 12P to BD
H02308039	AMD-357E IBP Adapter Cable, Mindray 12P to B.Braun
H02308040	AMD-357D IBP Adapter Cable, Mindray 12P to Edwards
H02308041	AMD-357C IBP Adapter Cable, Mindray 12P to Utah
H02308042	AMD-357F IBP Adapter Cable, Mindray 12P to USB




• For Edan Patient Monitor

PN	Product Description
H02308037	AMD-357A IBP Adapter Cable, Edan 12P to Abbott
H02308038	AMD-357B IBP Adapter Cable, Edan 12P to BD
H02308039	AMD-357E IBP Adapter Cable, Edan 12P to B.Braun
H02308040	AMD-357D IBP Adapter Cable, Edan 12P to Edwards
H02308041	AMD-357C IBP Adapter Cable, Edan 12P to Utah
H02308042	AMD-357F IBP Adapter Cable, Edan 12P to USB



• For Comen Patient Monitor

PN	Product Description
H02308043	AMD-099A IBP Adapter Cable, Comen 12P to Abbott
H02308044	AMD-099B IBP Adapter Cable, Comen 12P to BD
H02308045	AMD-099E IBP Adapter Cable, Comen 12P to B.Braun
H02308046	AMD-099D IBP Adapter Cable, Comen 12P to Edwards
H02308047	AMD-099C IBP Adapter Cable, Comen 12P to Utah
H02308048	AMD-099F IBP Adapter Cable, Comen 12P to USB




• For Biolight Patient Monitor

PN	Product Description
H02308049	AMD-033A IBP Adapter Cable, Biolight 4P to Abbott
H02308050	AMD-033B IBP Adapter Cable, Biolight 4P to BD
H02308051	AMD-033E IBP Adapter Cable, Biolight 4P to B.Braun
H02308052	AMD-033D IBP Adapter Cable, Biolight 4P to Edwards
H02308053	AMD-033C IBP Adapter Cable, Biolight 4P to Utah
H02308054	AMD-033F IBP Adapter Cable, Biolight 4P to USB



• For Datex-Ohmeda Patient Monitor

PN	Product Description
H02308061	AMD-012A IBP Adapter Cable, Datex-Ohmeda 10P to Abbott
H02308062	AMD-012B IBP Adapter Cable, Datex-Ohmeda 10P to BD
H02308063	AMD-012E IBP Adapter Cable, Datex-Ohmeda 10P to B.Braun
H02308064	AMD-012D IBP Adapter Cable, Datex-Ohmeda 10P to Edwards
H02308065	AMD-012C IBP Adapter Cable, Datex-Ohmeda 10P to Utah
H02308066	AMD-012F IBP Adapter Cable, Datex-Ohmeda 10P to USB

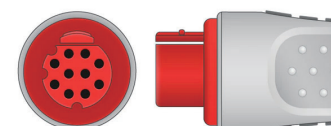


• For Infinium Medical Patient Monitor

PN	Product Description
H02308085	AMD-037A IBP Adapter Cable, Infinium Omni III Monitor 5P to Abbott
H02308086	AMD-037B IBP Adapter Cable, Infinium Omni III Monitor 5P to BD
H02308087	AMD-037E IBP Adapter Cable, Infinium Omni III Monitor 5P to B.Braun
H02308088	AMD-037D IBP Adapter Cable, Infinium Omni III Monitor 5P to Edwards
H02308089	AMD-037C IBP Adapter Cable, Infinium Omni III Monitor 5P to Utah
H02308090	AMD-037F IBP Adapter Cable, Infinium Omni III Monitor 5P to USB




• For Kontron Patient Monitor

PN	Product Description
H02308067	AMD-014A IBP Adapter Cable, Kontron 12P to Abbott
H02308068	AMD-014B IBP Adapter Cable, Kontron 12P to BD
H02308069	AMD-014E IBP Adapter Cable, Kontron 12P to B.Braun
H02308070	AMD-014D IBP Adapter Cable, Kontron 12P to Edwards
H02308071	AMD-014C IBP Adapter Cable, Kontron 12P to Utah
H02308072	AMD-014F IBP Adapter Cable, Kontron 12P to USB

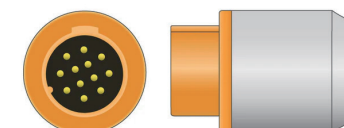

• For Spacelabs Patient Monitor

PN	Product Description
H02308055	AMD-075A IBP Adapter Cable, Spacelabs 10P to Abbott
H02308056	AMD-075B IBP Adapter Cable, Spacelabs 10P to BD
H02308057	AMD-075E IBP Adapter Cable, Spacelabs 10P to B.Braun
H02308058	AMD-075D IBP Adapter Cable, Spacelabs 10P to Edwards
H02308059	AMD-075C IBP Adapter Cable, Spacelabs 10P to Utah
H02308060	AMD-075F IBP Adapter Cable, Spacelabs 10P to USB

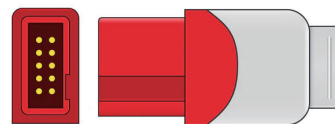


*For other customization needs, please contact Hisern's sales for details.

IBP Transducer Holder

• IBP Transducer Fixing Holder

PN	Product Description
H02309051	IBP Transducer Fixing Holder
H02309052	IBP Transducer Fixing Holder Plate

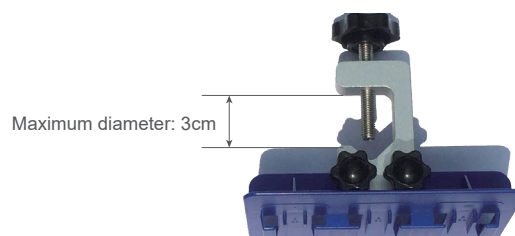

HISERN

Web: www.hisern.com/en

E-mail: sales@hisern.com / info@hisern.com

Tel: +86 0755-86660662

© 2024 Zhejiang Haisheng Medical Device Co., Ltd. All rights are reserved.

Zhejiang Haisheng Medical Device Co., Ltd. reserves the right to make changes in specifications and/or to discontinue any product at any time without notice or obligation and will not be liable for any consequences resulting from the use of this publication.

HISERNCGQ00120240001



LinkedIn



Website